0 GAMMA RAY api units 150	5"	0.2 1.0 10 100 1000 SPHERICALLY FOCUSSED RESISTIVITY
10 SPONTANEOUS POTENTIAL millivolts	Depths	0.2 1.0 10 100 1000 6FF40 INDUCTION RESISTIVITY ohms - m^2/m

REPEAT SECTION

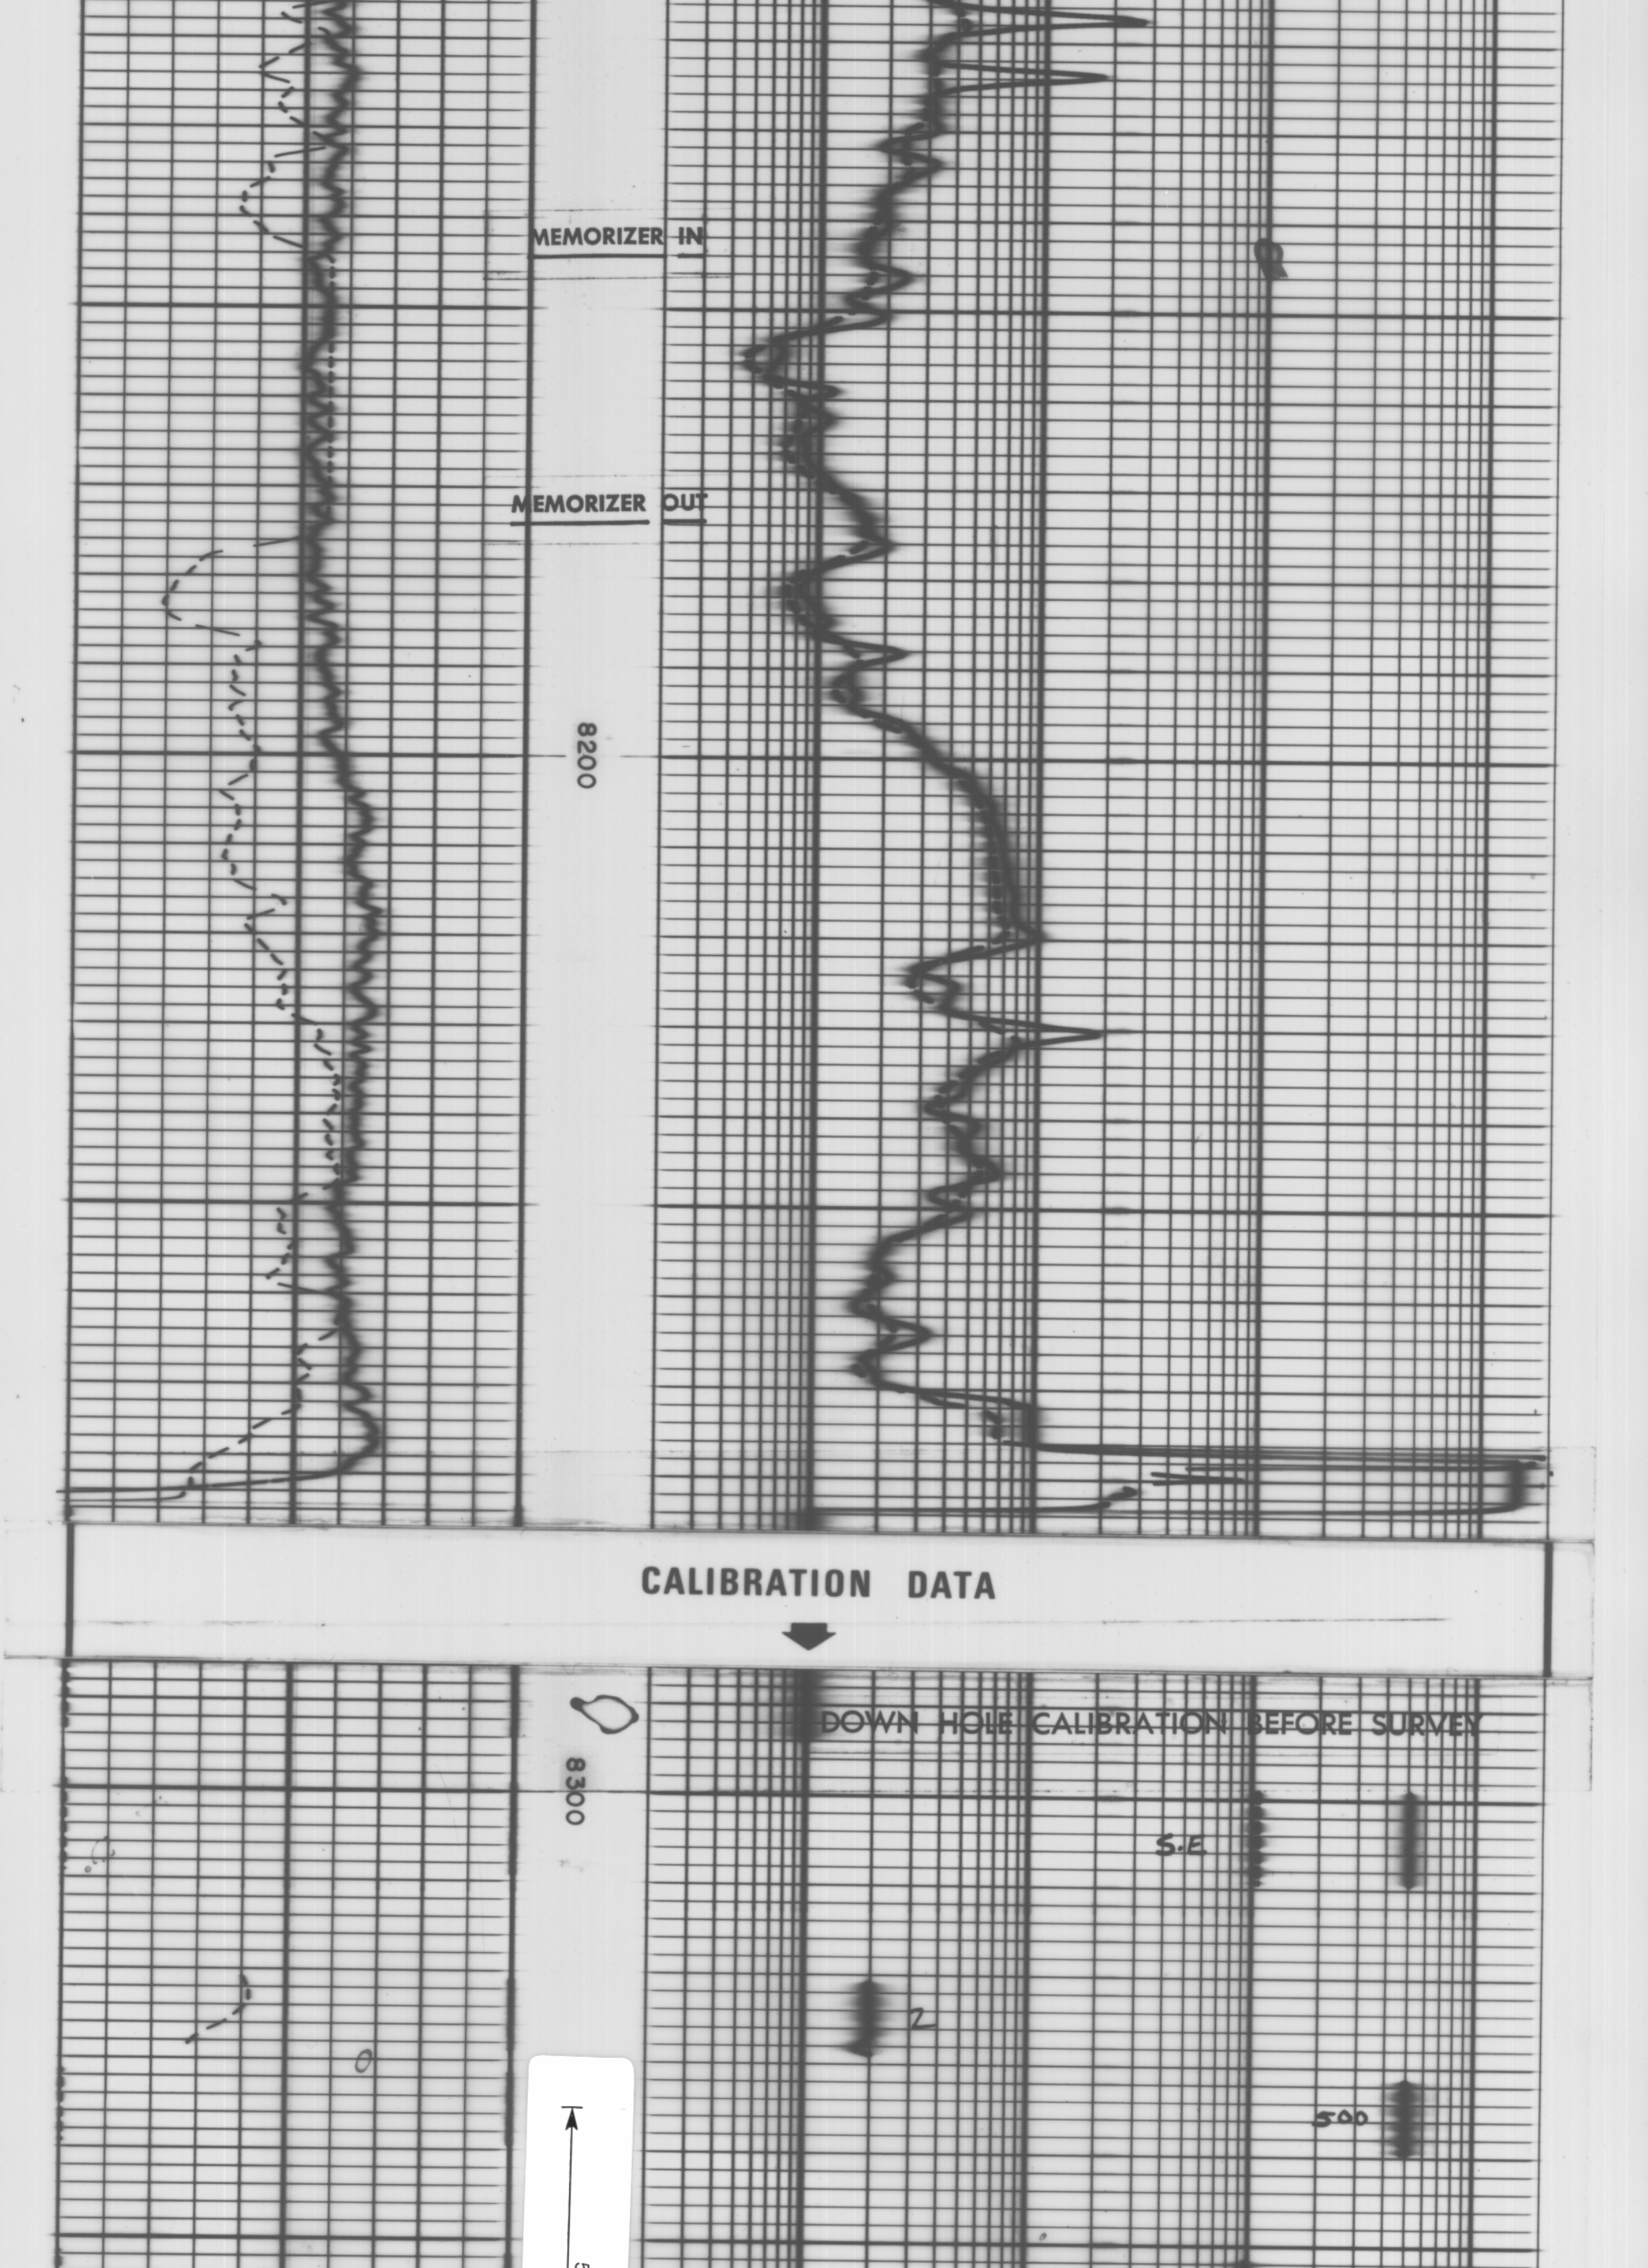

CALIBRATION DATA

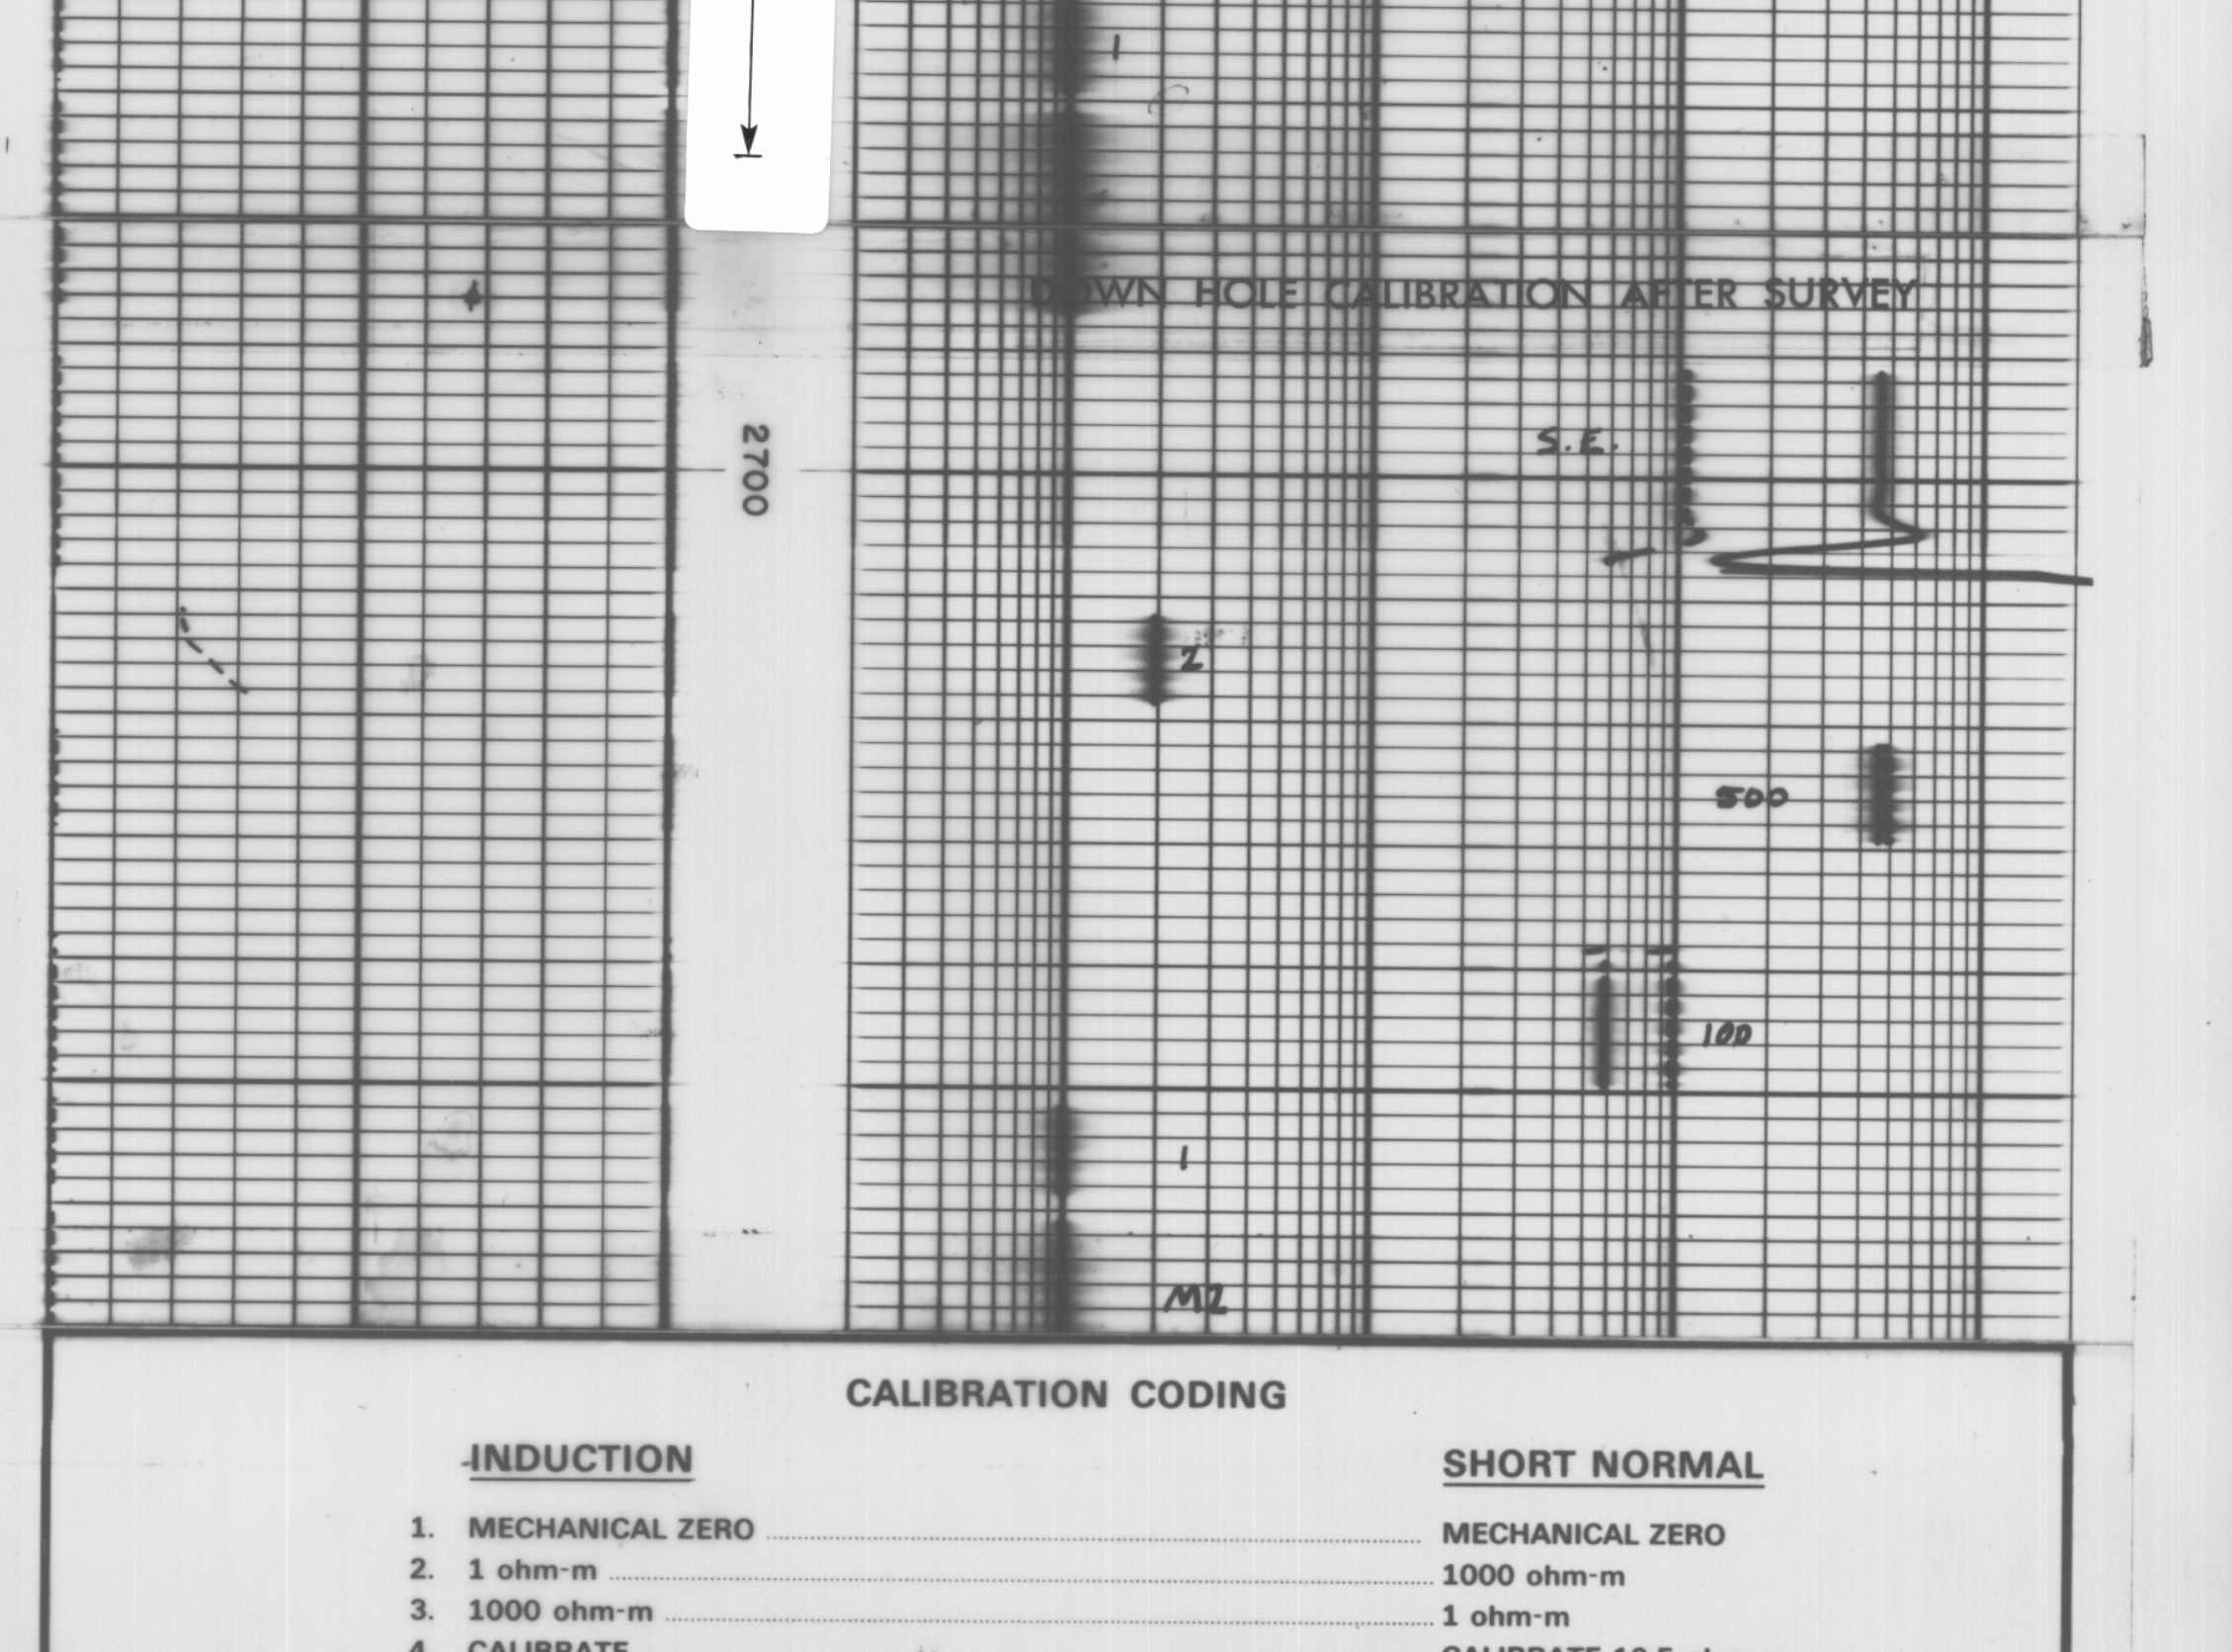

CALIBRATION CODING

	INDUCTION	SHORT NORMAL
1.	MECHANICAL ZERO	MECHANICAL ZERO
2.	1 ohm-m	1000 ohm-m
3.	1000 ohm-m	1 ohm-m
4.	CALIBRATE	CALIBRATE 10.5 ohm-m
5.	SONDE ERROR	ELECTRICAL ZERO 1 ohm-m
6.	DIODE ERROR	ELECTRICAL ZERO 1 ohm-m
7.	MEMORIZER CALIBRATION	CALIBRATE 10.5 ohm-m
8.	ZERO SIGNAL IN AIR	SURFACE CALIBRATION ONLY
9.	TEST LOOP	SURFACE CALIBRATION ONLY

Schlumberger

INDUCTION ELECTRICAL LOG